


Example Preterm Labor Protocol

HOLOGIC®

Patients with symptoms of preterm labor 24⁰ - 34⁶ weeks

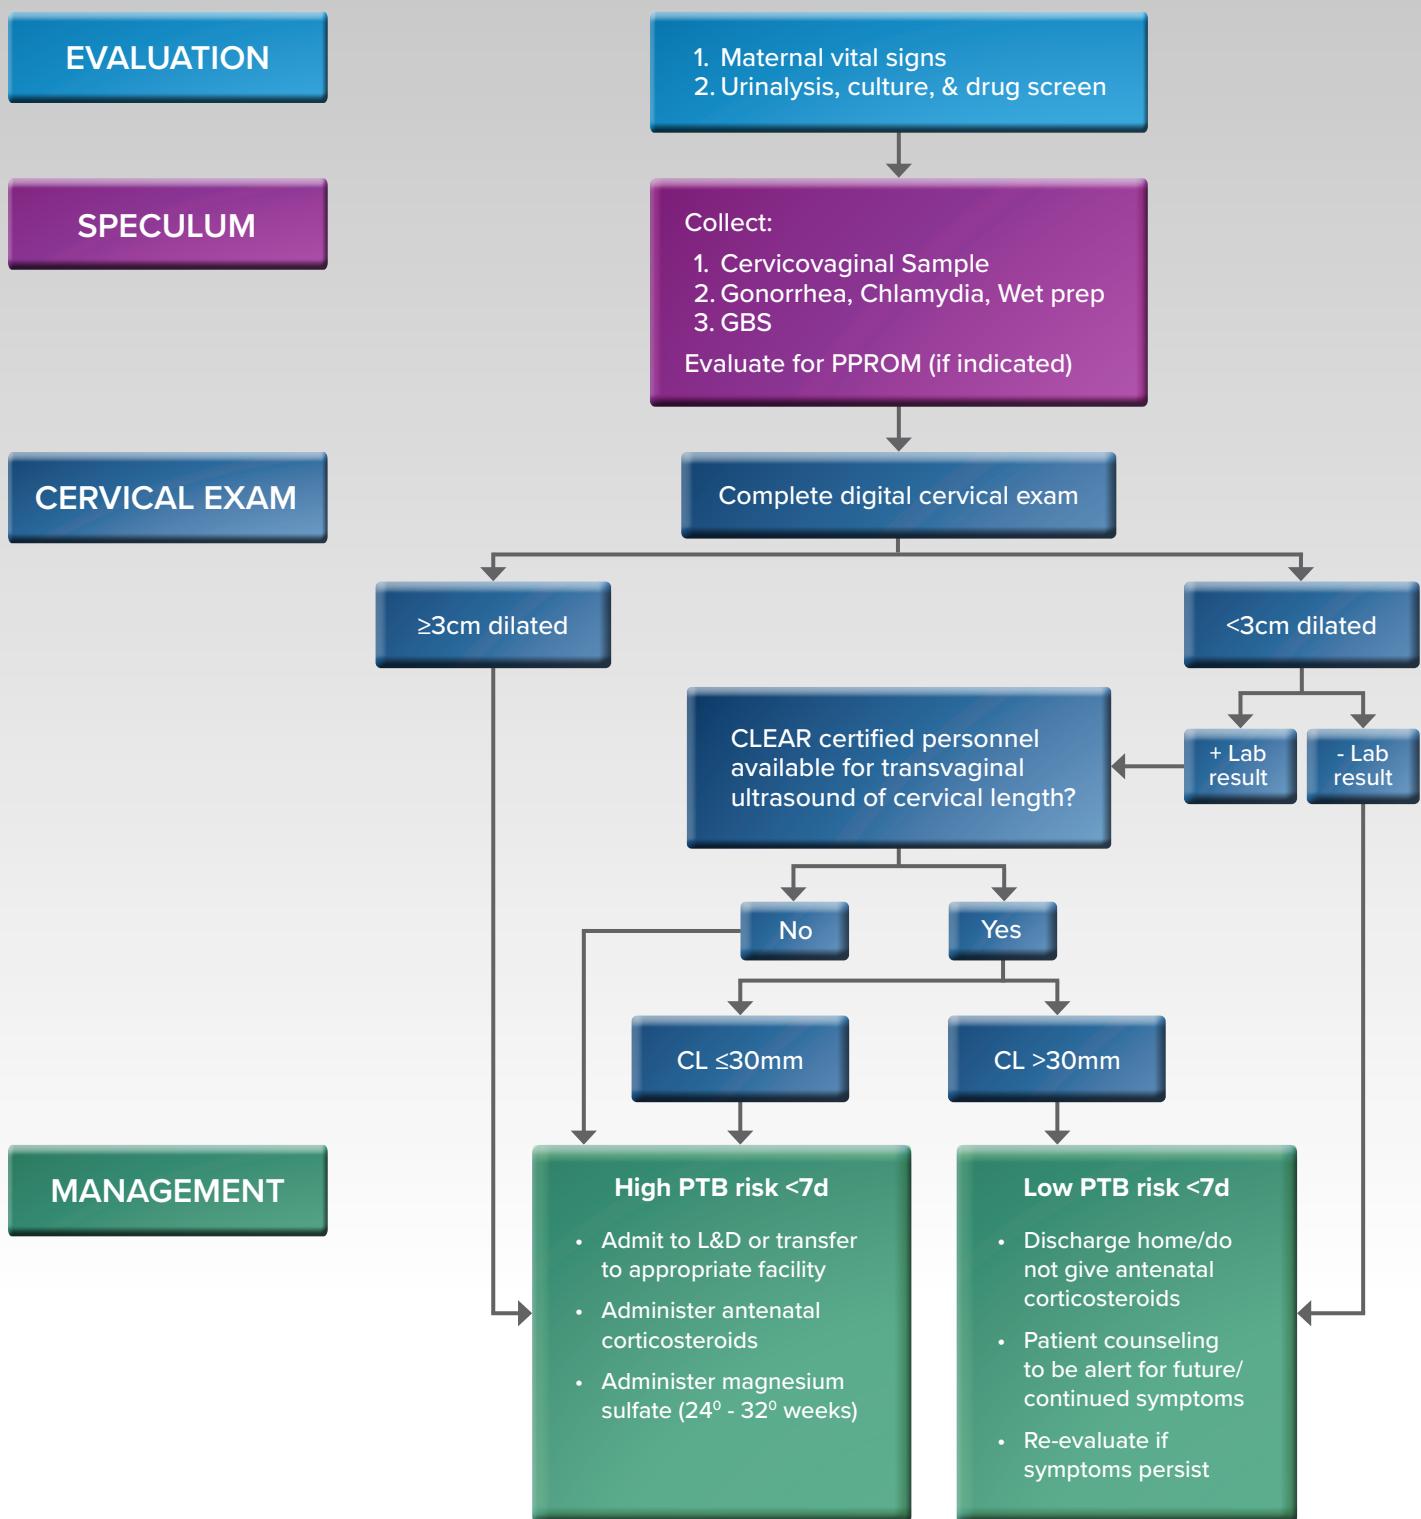

The Perinatal Quality Foundation initiated the CLEAR program (Cervical Length Education and Review) in 2011 to develop consensus on the standard criteria for sonographic cervical measurements during pregnancy. Practitioners who complete the lectures and pass the examination and image review receive verification that they have completed the CLEAR program.

MED-00888-001 Rev. 001 © 2024 Hologic, Inc. All rights reserved. Hologic, and associated logos are trademarks and/or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries. This is a general information tool for medical professionals and is not a complete representation of the product(s) Instruction for Use (IFU) or Package Insert, and it is the medical professionals' responsibility to follow the IFU or Package Insert. The information provided may suggest a particular technique or protocol however the information is not and should not be construed as medical advice. It is the sole responsibility of the medical professional to determine which technique or protocol is appropriate. At all times, clinicians remain responsible for utilizing sound patient evaluation and selection practices and for complying with applicable local, state, and federal rules and regulations. In no event shall Hologic be liable for damages of any kind resulting from your use of the information. Because Hologic materials are distributed through websites, eBroadcasts and tradeshows, it is not always possible to control where such materials appear. For specific information on what products are available for sale in a particular country, please contact your local Hologic representative or write to diagnostic.solutions@hologic.com